

Intramedullary  
Tibial Preparation  
Primary Total Knee Arthroplasty





# LEGION<sup>◊</sup> Total Knee System

## Intramedullary tibial preparation

### Contents

Introduction .....	2
IM tibial highlights .....	3
Preoperative planning .....	4
Instrument assembly.....	5
IM tibial preparation .....	6
Tibial sizing.....	9
Component trialing.....	11
Implantation .....	13
Appendix A .....	15
Appendix B.....	16

### Nota Bene

The technique description herein is made available to the healthcare professional to illustrate the authors' suggested treatment for the uncomplicated procedure. In the final analysis, the preferred treatment is that which addresses the needs of the patient.

Additional LEGION Total Knee System surgical technique brochures are available for the other LEGION Components.

# Introduction

The LEGION® Total Knee System has been designed to offer the orthopaedic surgeon solutions to address intraoperative situations. Implant function is directly related to accurate surgical technique. LEGION instrumentation has been developed to be an easy-to-use system that will assist the surgeon in obtaining accurate and reproducible knee alignment.

The instrumentation can be used in minimally invasive or standard exposures. While it has been the designers' objective to develop accurate, easy-to-use instrumentation, each surgeon must evaluate the appropriateness of the following technique based on his or her medical training, experience and patient evaluation.

# IM tibial highlights

Place the intramedullary alignment assembly on the tibia. The alignment rod should align with the medial third of the tibial tubercle. Impact assembly.



Attach the tibial stylus to the tibial cutting block and lower the cutting block until the stylus touches the low point on the least affected side of the tibia. Once the resection level is determined, insert pins to secure and remove alignment assembly.



Resect the proximal tibia.



Size the tibia.



## Final preparation

After trial ROM and alignment checks, select the appropriate trial fin punch and punch through the trial.



Seat the tibial implant with the tibial impactor.



Attach the articular inserter/extractor to the tibial tray (for standard inserts). Lift inserter superiorly until the anterior lip of the insert is fully seated.




# Preoperative planning

Determine the angle between the anatomical and the mechanical axes. This measurement will be used intraoperatively to select the appropriate valgus angle so that correct limb alignment is restored. (Beware of misleading angles in knees with a flexion contracture or rotated lower extremities.) The T-template provided as part of the LEGION® templates will help in this determination.



*Tip: Many surgeons prefer to simply select a standard angle for the distal femoral cut (ie, 5°, 6° or 7°) based on the patient and surgical experience.*

## Recommended sawblades

1.27 Sawblade (for standard blocks)  
Cutting thickness and blade thickness should be 0.050" or 1.27mm.

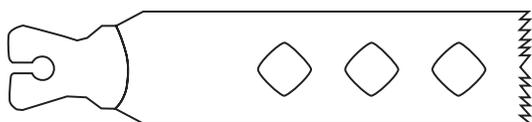

1.35 Sawblade (for MIS blocks)  
Cutting thickness and blade thickness should be 0.053" or 1.35mm.

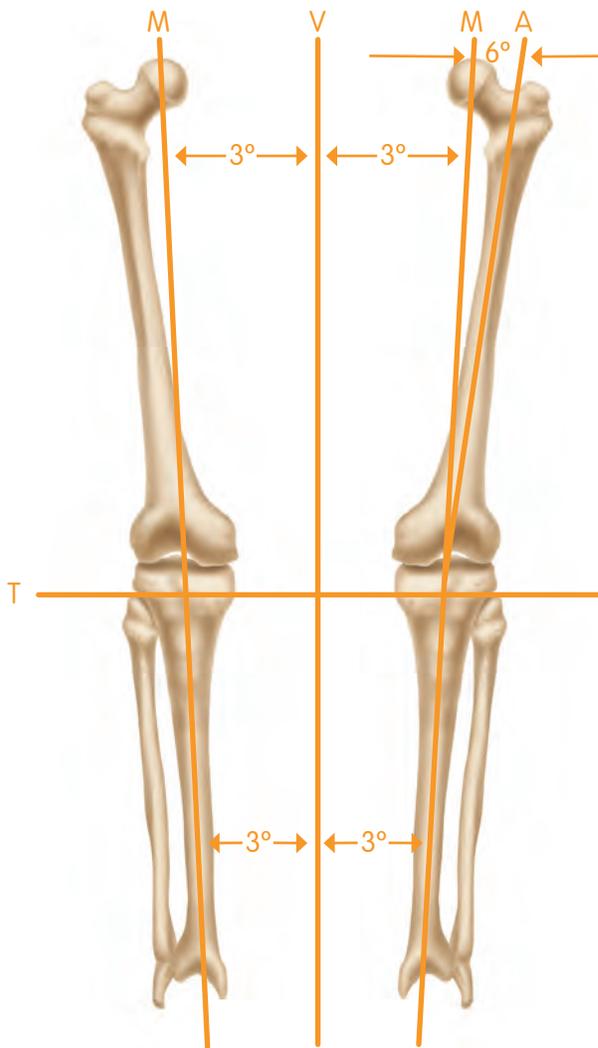

M = Mechanical Axis

A = Anatomical Axis

T = Transverse Axis

V = Vertical Axis

# Instrument assembly

## Intramedullary tibial alignment guide

- 1 Insert the external rod of the Intramedullary tibial alignment guide through the hole on the correct left or right tibial cutting block and lock the cam (Figure 1).
- 2 Attach the T-handle to the IM rod and pass it through the cannulated alignment sleeve on the alignment assembly (Figure 2).

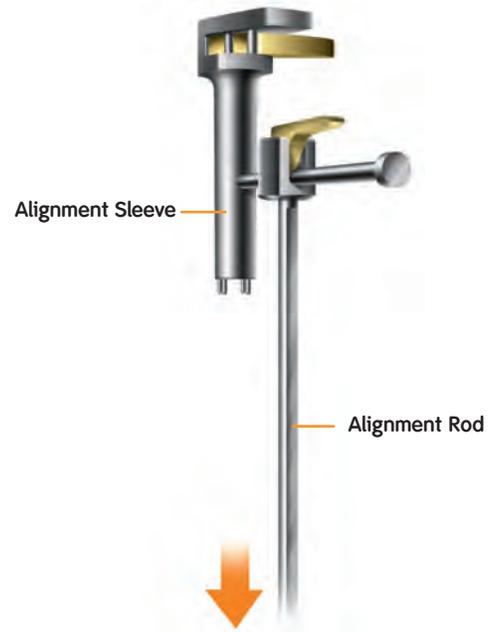


Figure 1



Figure 2

T-handle  
7111-0080

Tibial Cutting Block  
Left 7144-1136  
Right 7144-1137

IM Alignment  
Guide 7144-0200

IM Rod  
Short 7144-0006  
Long 7144-0004

# IM tibial preparation

1 Make a 9.5mm pilot hole into the tibial canal (Figure 3). A preliminary resection of the tibial spine may facilitate seating of the tibial drill guide onto the proximal tibia.



Figure 3

2 Slowly insert the IM rod into the tibial canal.

3 Assess rotation of the intramedullary tibial alignment guide. Rotational alignment is critical due to the 3° posterior sloped cut. The alignment rod of the intramedullary tibial alignment assembly should align with the medial third of the tibial tubercle (Figure 4).



Figure 4

4 Impact the proximal end of the cannulated alignment sleeve to drive the distal spikes into the proximal tibia to lock rotational alignment (Figure 5).

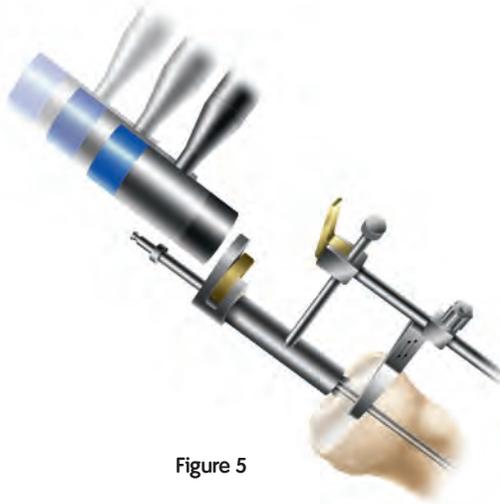


Figure 5

---

<b>IM Drill</b>	<b>Tibial Cutting Block</b>	<b>IM Alignment</b>	<b>IM Rod</b>
7144-0002	Left 7144-1136	Guide 7144-0200	Short 7144-0006
	Right 7144-1137		Long 7144-0004

# Tibial resection

- 1 Attach the tibial stylus to the tibial cutting block by inserting the stylus foot into the cutting slot.
- 2 Lower the cutting block until the stylus touches the low point on the least affected side of the tibia (Figure 6). The stylus can be adjusted for a 1-13mm tibial resection by twisting the knob on top of the stylus. If the affected side of the tibia is to be used as a reference, the stylus may be adjusted for a 1-9mm resection level.
- 3 Pin the tibial cutting block to the tibia by inserting pins first through the central holes; then the oblique hole.

Tip: Pinning through the central holes marked 0mm with smooth pins will allow the block to be moved +2mm should additional resection be required (Figure 7).

Tip: A 9mm resection is recommended since 9mm of metal and plastic is the thinnest available component.

Tip: To do an extramedullary alignment check, place the extramedullary alignment rod through the tibial cutting block.



Figure 6



Figure 7

---

Tibial Stylus	Tibial Cutting Block	Alignment Rod
7144-1143	Left 7144-1136	7144-1148
	Right 7144-1137	

- 4 To remove the assembly:  
Use the universal extractor leaving the cutting block on the anterior tibia (Figure 8) after loosening the thumbscrew.
- 5 Cut the tibia by first directing the blade in the posterior direction and then laterally (Figure 9).
- 6 Check alignment and balance with spacer block and rod (Figures 10 and 11). Balance ligaments in standard fashion.

Tip: If you are using a spacer block from the GENESIS® II set, use the extension end to check both flexion and extension spaces.



Figure 8



Figure 9



Figure 10



Figure 11

Universal Extractor (Slap Hammer)	Spacer Block original two-sided)	Spacer Block (new one-sided)	Tibial Cutting Block Left	Alignment Rod
7144-0366	7144-0828	7144-1265	7144-1136	7144-1148
			Right 7144-1137	

# Tibial sizing

## Option A – stemless tibial trials

1 Attach a quick-connect handle to a stemless trial one size below the femoral component size and place on the cut tibia to assess coverage (Figure 12). As needed, additional sizes should be templated using the stemless trials.

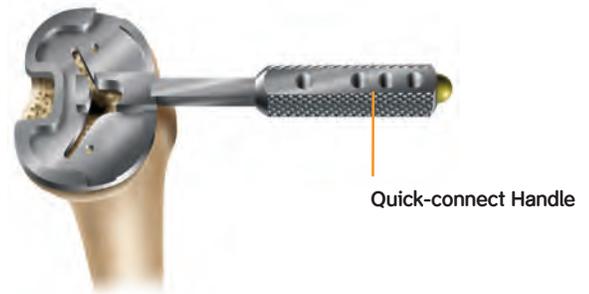


Figure 12

2 Once the appropriate size is determined, pin the medial size of the selected stemless trial with a short headed pin.

3 Place a trial insert into the stemless tibial trial tray and perform a trial range of motion to allow the baseplate to center on the femoral trial. (As a secondary check, the surgeon may pass the alignment rod through the quick-connect handle to assess alignment) (Figure 13). Pin the lateral side of the trial.

**Tip:** After putting the knee through a trial ROM, the surgeon should note the proper rotation of the trial tibial component on the proximal tibia and mark the tibia for future reference.

**Tip:** The center-line marks on the femoral and tibial trial components should line up.

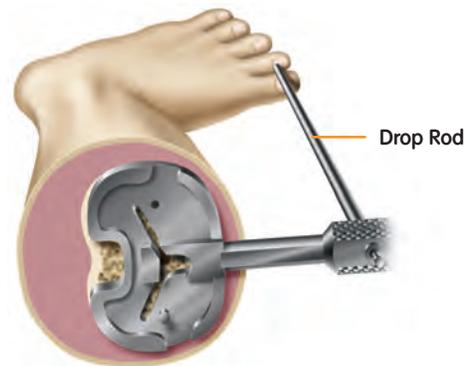


Figure 13

4 Using the tibial fin/stem punch, rotational alignment may be set now or at the time of trial placement.

**Tip:** In the case of sclerotic bone, first drill for the stem using the 11mm tibial drill. Begin the fin slot with a burr or thin sawblade before using the fin punch to prevent tibial fracture.

Quick-connect Handle	Stemless Trials		Fin/Stem Punch	11mm Tibial Drill
	Left	Right		
7144-0044	sz 1 7143-0161	sz 1 7143-0177	sz 1-2 7144-9991	7144-0040
7144-0045	sz 2 7143-0163	sz 2 7143-0179	sz 3-4 7144-9993	
	sz 3 7143-0165	sz 3 7143-0181	sz 5-6 7144-9995	
	sz 4 7143-0167	sz 4 7143-0183	sz 7-8 7144-9997	
	sz 5 7143-0169	sz 5 7143-0185		
	sz 6 7143-0171	sz 6 7143-0187		
	sz 7 7143-0173	sz 7 7143-0189		
	sz 8 7143-0175	sz 8 7143-0191		

## Option B – stemmed tibial trials

- 1 Place a tibial drill guide one size below the femoral component size on the cut tibia to assess coverage. As needed, additional sizes should be templated (Figure 14).
- 2 Once the tibial drill guide has been centralized on the proximal tibia, pin the drill guide in place. Retract the gold collar on the drill guide handle and insert the 11mm tibial collet.
- 3 With the 11mm tibial collet in place, drill with the 11mm tibial drill (Figure 15) and punch with the 11mm tibial punch (Figure 16).
- 4 Remove the tibial drill guide.
- 5 Place the stemmed tibial trial into the prepared hole.
- 6 Using the tibial fin punch, rotational alignment may be set now or at the time of trial placement.



Figure 14



Figure 15



Figure 16

**Tip:** After putting the knee through a trial ROM, the surgeon should note the proper rotation of the trial tibial component on the proximal tibia and mark the tibia for future reference.

**Tip:** The center-line marks on the femoral and tibial trial components should line up.

### 11mm Tibial Drill 7144-0040

#### Stem Trials

##### Left

sz 1	7143-0160
sz 2	7143-0162
sz 3	7143-0164
sz 4	7143-0166
sz 5	7143-0168
sz 6	7143-0170
sz 7	7143-0172
sz 8	7143-0174

##### Right

sz 1	7143-0176
sz 2	7143-0178
sz 3	7143-0180
sz 4	7143-0182
sz 5	7143-0184
sz 6	7143-0186
sz 7	7143-0188
sz 8	7143-0190

### Fin/Stem Punch

sz 1-2	7144-0264
sz 3-4	7144-0266
sz 5-6	7144-0268
sz 7-8	7144-0270

### 11mm Tibial Punch

7144-0262

# Component trialing

- 1 Use the appropriate insert trial (begin with a 9mm trial) to determine stability and alignment.
- 2 Perform a trial range of motion. The alignment marks on the front of the femoral and tibial trials should line up (Figure 17). The quick-connect handle may be attached to the tibial trial and used to set the appropriate rotational alignment.

Option: Extend the knee fully with the handle attached to the tibial trial. Pass the extramedullary rod through the handle to assess full leg alignment (Figure 18).

Tip: The technique of tibial trial, then femoral trial and then trial insert works for all LEGION® primary inserts *except* the dished inserts. For the deep dished, insert the trial bearing BEFORE the femoral trial.



Figure 17



Figure 18

CR Insert Trials	PS High Flex Insert Trials	Deep Dished Insert Trials	Insert Trial Spacers	Constrained Insert Trials
<b>9mm</b>	<b>9mm</b>	<b>9mm</b>	<b>13mm</b>	<b>9mm</b>
sz 1-2 7143-0880	sz 1-2 7143-0401	sz 1-2 7143-0454	sz 1-2 7143-0324	sz 1-2 7144-0471
sz 3-4 7143-0490	sz 3-4 7143-0408	sz 3-4 7143-0766	sz 3-4 7143-0226	sz 3-4 7144-0473
sz 5-6 7143-0500	sz 5-6 7143-0415	sz 5-6 7143-0778	sz 5-6 7143-0228	sz 5-6 7144-0475
sz 7-8 7143-0510	sz 7-8 7143-0422	sz 7-8 7143-0789	sz 7-8 7143-0230	sz 7-8 7144-0477
<b>11mm</b>	<b>11mm</b>	<b>11mm</b>	<b>15mm</b>	<b>11mm</b>
sz 1-2 7143-0882	sz 1-2 7143-0402	sz 1-2 7143-0456	sz 1-2 7143-0332	sz 1-2 7143-0962
sz 3-4 7143-0492	sz 3-4 7143-0409	sz 3-4 7143-0768	sz 3-4 7143-0234	sz 3-4 7143-0524
sz 5-6 7143-0502	sz 5-6 7143-0416	sz 5-6 7143-0780	sz 5-6 7143-0236	sz 5-6 7143-0538
sz 7-8 7143-0512	sz 7-8 7143-0423	sz 7-8 7143-0791	sz 7-8 7143-0238	sz 7-8 7143-0538
<b>PS Insert Trials</b>	<b>CR Deep Flex Insert Trials</b>		<b>18mm</b>	
<b>9mm</b>	<b>9mm</b>		sz 1-2 7143-0340	
sz 1-2 7143-0901	sz 1-2 7143-0442		sz 3-4 7143-0242	
sz 3-4 7143-0815	sz 3-4 7143-0444		sz 5-6 7143-0244	
sz 5-6 7143-0829	sz 5-6 7143-0446		sz 7-8 7143-0246	
sz 7-8 7143-0844	sz 7-8 7143-0448		<b>21mm</b>	
<b>11mm</b>	<b>11mm</b>		sz 1-2 7143-0348	
sz 1-2 7143-0903	sz 1-2 7143-0443		sz 3-4 7143-0250	
sz 3-4 7143-0817	sz 3-4 7143-0445		sz 5-6 7143-0252	
sz 5-6 7143-0831	sz 5-6 7143-0447		sz 7-8 7143-0254	
sz 7-8 7143-0846	sz 7-8 7143-0449		<b>25mm</b>	
			sz 1-2 7143-0356	
			sz 3-4 7143-0258	
			sz 5-6 7143-0260	
			sz 7-8 7143-0262	

3 Mark correct tibial rotational alignment on the anterior tibia using a cautery knife (Figure 19).

4 Select the appropriate tibial fin punch to prepare the fins and punch through the tibial trial (Figure 20).

Tip: If the tibial bone is sclerotic, begin the fin slot with a burr or thin sawblade before using the fin punch to prevent tibial fracture.

5 Perform a trial range of motion to assess implant function (Figure 21).

6 Remove the tibial trial.

Precaution: Implants are not designed to be used as trial components. Their use as trial components may expose the implant's cementing surface to body fluid and/or fat. This exposure would contaminate the implant/cement interface and potentially compromise implant fixation by reducing cement bonding strength. This may cause premature implant loosening, leading to implant revision.



Figure 19



Figure 20

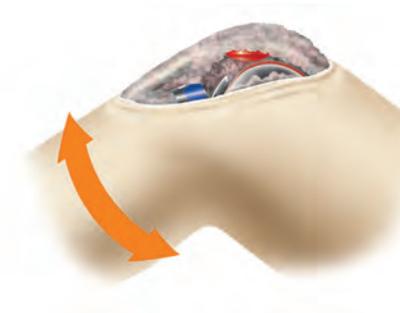


Figure 21

# Implantation

- 1 Apply cement on the proximal tibia and/or the implant and seat the tibial implant with the tibial impactor (Figure 22). Remove excess cement.

## **Cruciate-retaining, dished and posterior stabilized insert placement**

- 2 Determine the correct articular insert thickness.
- 3 Clear any debris from the locking mechanism and slide the insert into the tibial baseplate engaging the locking mechanism. For the PS insert, begin insertion in flexion and extend the leg to engage the locking mechanism.
- 4 Attach the articular inserter/extractor to the tibial tray. Lift the inserter superiorly until the anterior lip of the articular insert is fully seated (Figure 23).



Figure 22



Figure 23

---

Tibial Base  
Impactor  
7144-0192

Articular Inserter/  
Extractor  
7144-0194

## PS high flex and CR deep flex insert placement

- 1 Attach the appropriately sized impactor head (either 1-2 or 3-8) to the impactor handle.
- 2 Position the knee in approximately 90° flexion.
- 3 Align the articular insert with the locking mechanism of the tibial baseplate.
- 4 Push the insert posteriorly until the top of the anterior rail of the baseplate is visible.
- 5 Place the bumper on the anterior chamfer of the insert. The mating surfaces should be very conforming (Figures 24-25).
- 6 Impact the handle until the insert is fully seated.



Figure 24



Figure 25

**MIS Note:** To use the PS high flexion insert in minimally invasive surgery, please see the technique described in Appendix A.

---

High-flex Impactor Head	High-flex Impactor Handle	Bone Cement
sz 1-2 7144-1553	7144-1552	
sz 3-8 7144-1554		

# Appendix A

## LEGION® PS high flex insert impaction technique for MIS

When using the PS high flex insert in a minimally invasive procedure, the femoral cam mechanism is likely to prevent the insert from fully seating into the locking mechanism while the knee is in flexion. To use the PS high flex insert in a MIS case:

- 1 Flex the knee to 90° and push the insert as far back as it will go posteriorly with the knee in flexion (Figure 26).

**Tip:** Lift the distal femur to prevent scratching of the posterior condyle of the component.

- 2 Placing your thumb on the anterior of the insert to hold it on the baseplate (Figure 27), move the knee into extension.
- 3 Use the impactor handle with the appropriately sized bumper to fully seat the insert and engage the anterior portion of the dovetail locking mechanism (Figure 28).



Figure 26

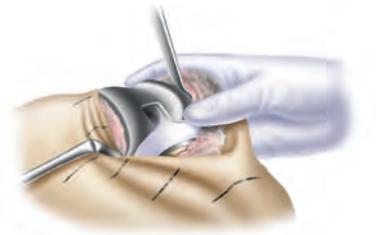


Figure 27



Figure 28

# Appendix B

## LEGION<sup>®</sup> articular insert interchangeability chart

	Femoral Size							
Insert Size	1	2	3	4	5	6	7	8
1-2 PS, DD, Con	●	●	●					
1-2 HFPS, CRDF	●	●	●	●				
3-4 PS, DD, Con		●	●	●	●			
3-4 HFPS, CRDF		●	●	●	●	●		
5-6 PS, DD, Con				●	●	●	●	
5-6 HFPS, CRDF				●	●	●	●	●
7-8 PS, DD, Con						●	●	●
7-8 HFPS, CRDF						●	●	●



**Orthopaedics**

Smith & Nephew, Inc.  
1450 Brooks Road  
Memphis, TN 38116  
USA

[www.smith-nephew.com](http://www.smith-nephew.com)  
[www.legionpower.com](http://www.legionpower.com)

Telephone: 1-901-396-2121  
Information: 1-800-821-5700  
Orders and Inquiries: 1-800-238-7538